

FIG. 1

Description of Schematic Diagram

- A. Color Beads DNA Microarray
- B. Illumination light source
- C. Cover Lid
- D. Light Deflector
- E. Lens
- F. Charge Coupled Device (CCD)
- G. Camera
- H. Computer control unit

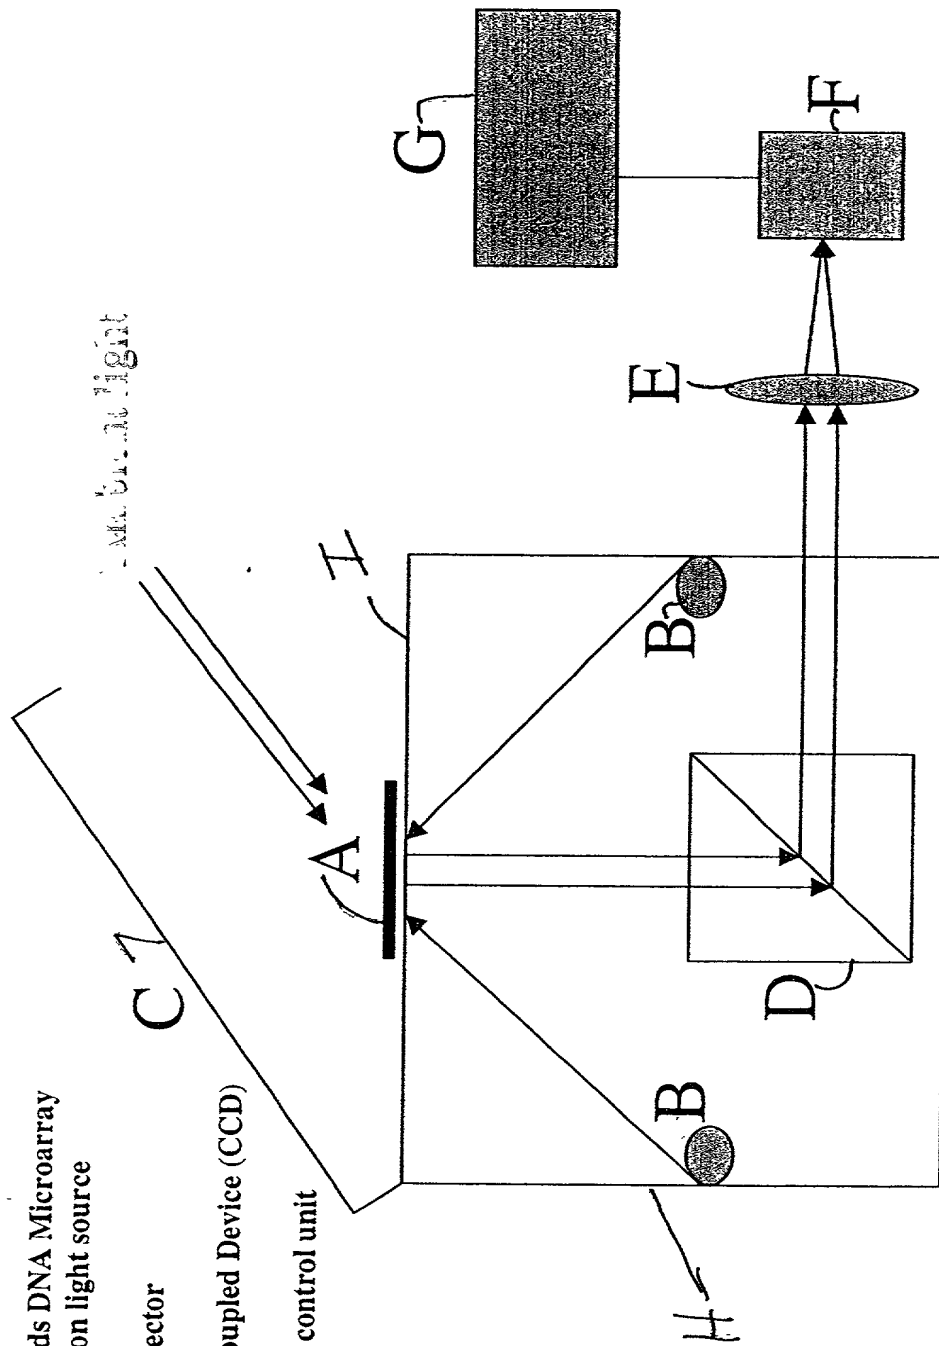


FIG. 2

Workflow Chart of Nucleic Acid Random Microarray Analysis System

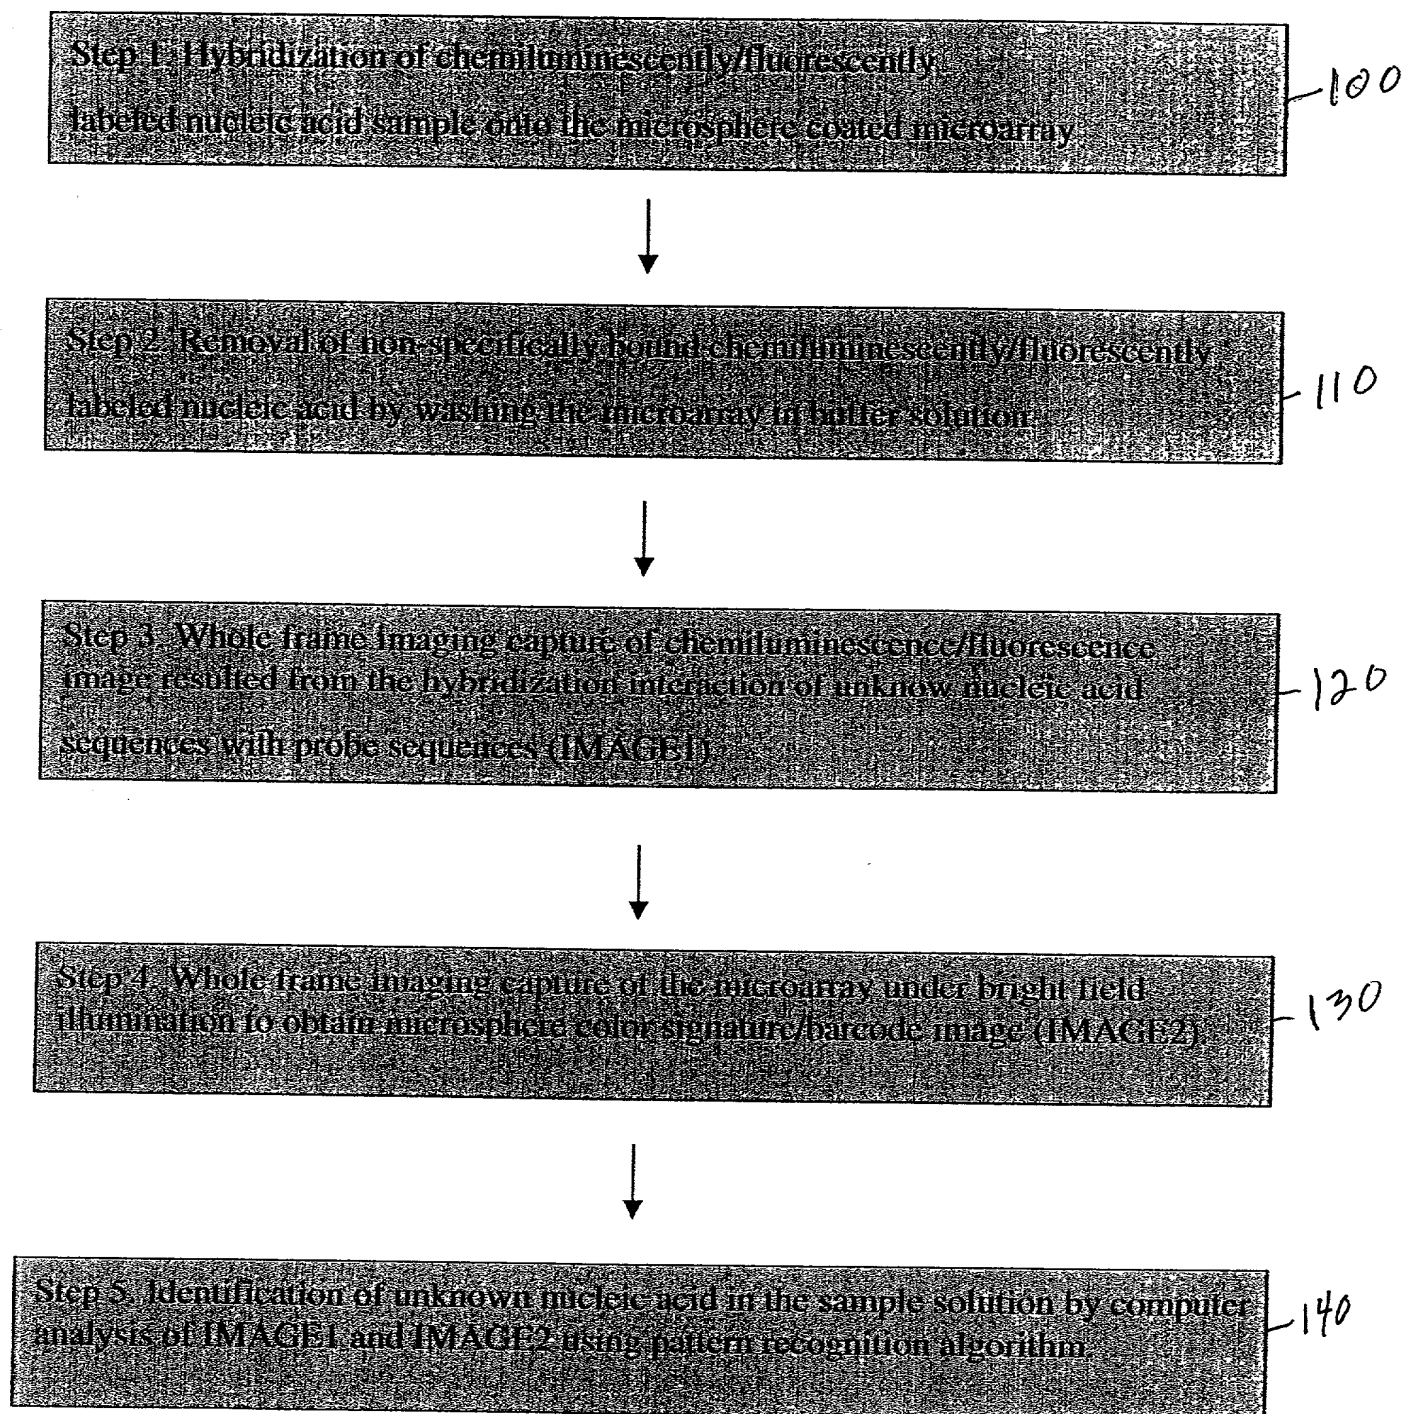


FIG. 3

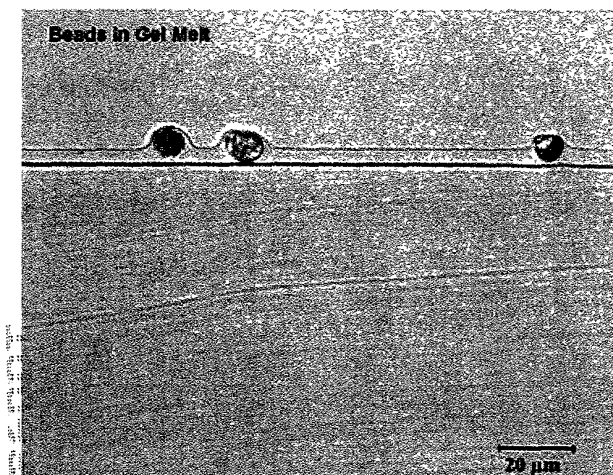


Fig 2A-

F. 1. 1. 1.

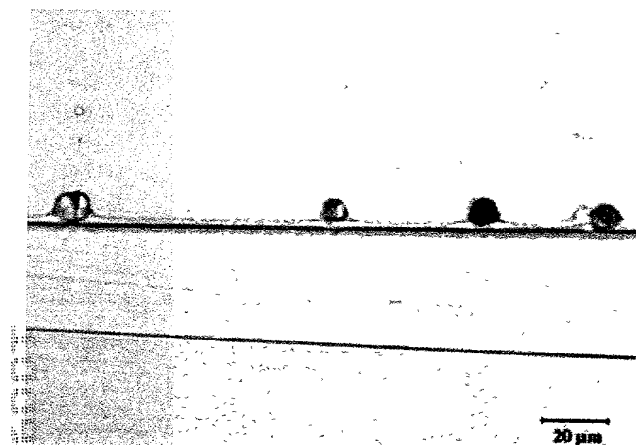


Fig 2B

Fig. 2B



20 μ m

Fig 2C
Fig 2C



Fig. 2D

1000

20 建築


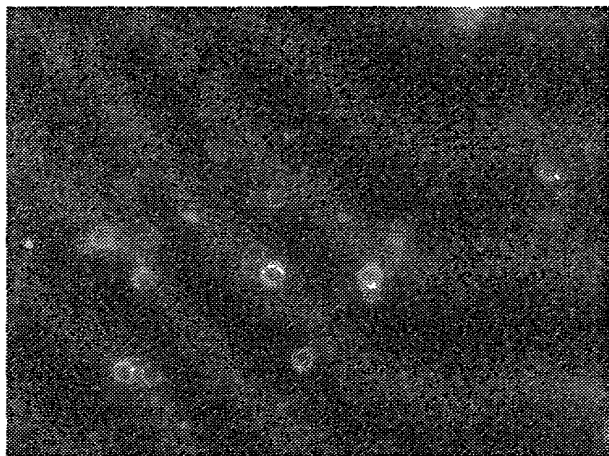


Fig 3A

1.5.20

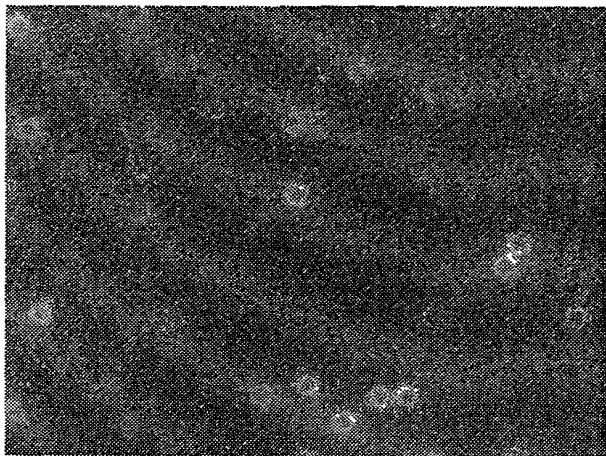

~~Fig. 3B~~

Fig. 3B

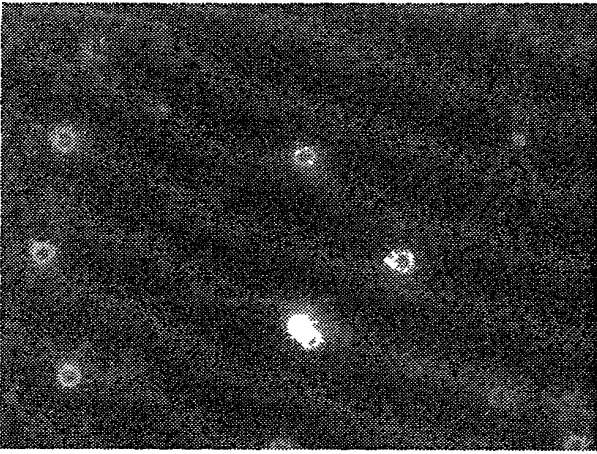


Fig. 3c

Fig. 3c

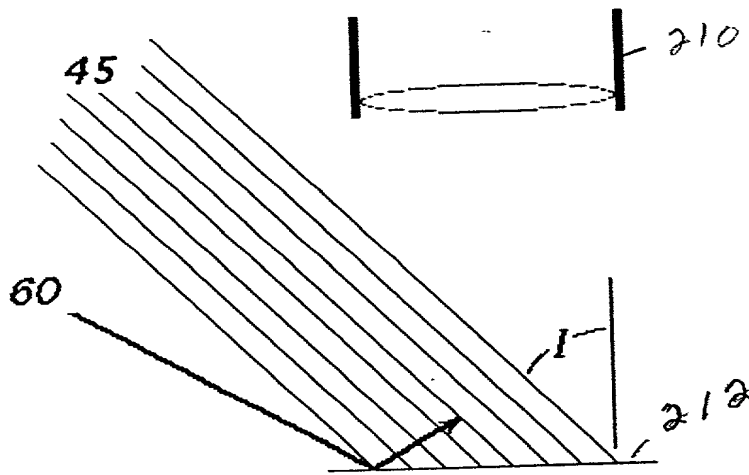


FIG. 6A

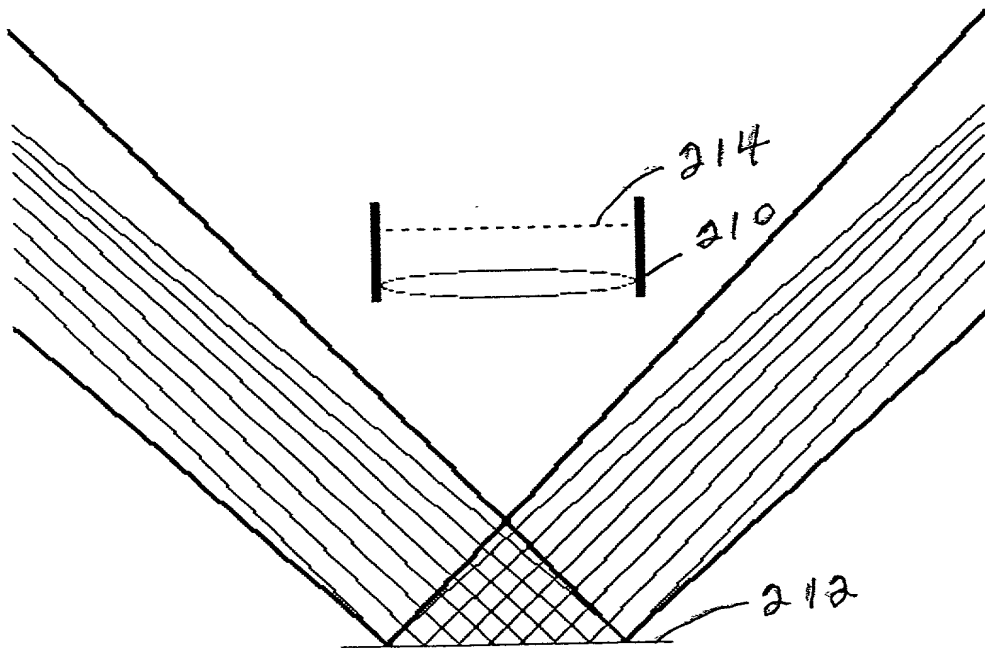


FIG. 6E

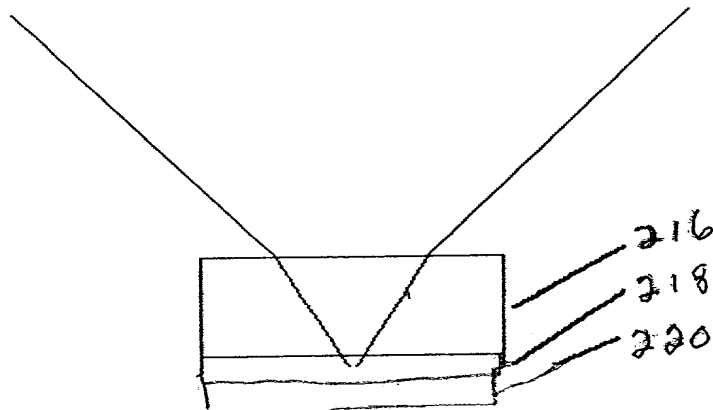


FIG. 6C